


Spectrum Point Pick Report

01/15/2018 08:23:29 AM

Data Set: **Transmittance (RCT3) Graph** - RawData

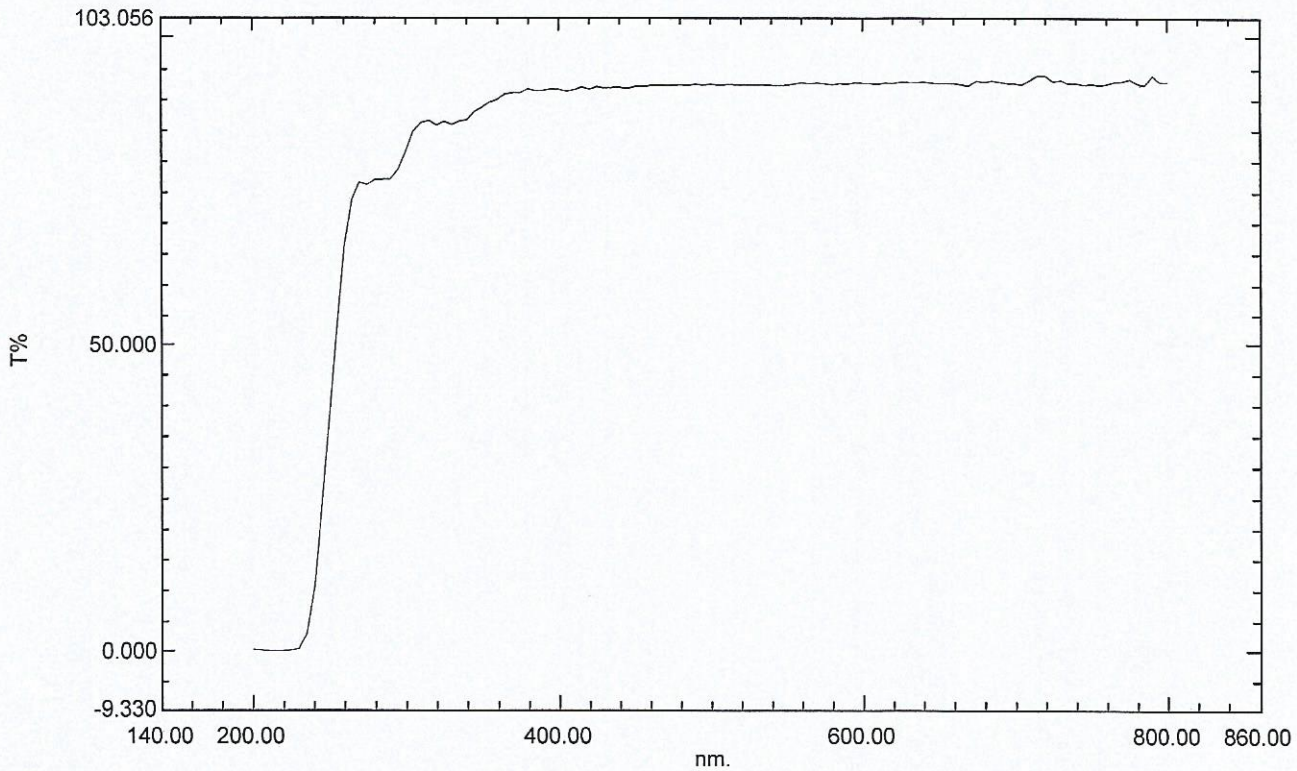

[Measurement Properties]
 Wavelength Range (nm.): 200.00 to 800.00
 Scan Speed: Fast
 Sampling Interval: 5.0
 Auto Sampling Interval: Disabled
 Scan Mode: Auto

No.	Wavelength	Transmittan	Description
1	300.00	81.235	
2			

[Instrument Properties]
 Instrument Type: UV-2600 Series
 Measuring Mode: Transmittance
 Slit Width: 2.0
 Accumulation time: 2.0 sec.
 Light Source Change Wavelength: 323.0 nm
 Detector Unit: External(2Detector)
 Detector Change Wavelength: 870.0 nm
 S/R Exchange: Normal
 Stair Correction: OFF

[Attachment Properties]
 Attachment: None

[Operation]
 Threshold: 0.0010000
 Points: 4
 InterPolate: Disabled
 Average: Disabled

[Sample Preparation Properties]
 Weight:
 Volume:
 Dilution:
 Path Length:
